

M1.(a) (i) Fluorescent screen A – converts X-ray (photon) to light (photons) / lower energy photon(s) 1

(ii) Photocathode – uses (energy of) each light photon to release an electron from surface of cathode

Do not allow converts light / photon into electron

1

(iii) Anodes – accelerate (released) electrons
focuses electron beams

Mention of negative anode disqualifies first mark awarded

Do not accept direct towards the screen as focussing

2

(iv) Fluorescent screen B – converts energy of electron(s) into (many) light (photons)

Do not allow converts electrons into light / photons

1

(b) Without Barium poor contrast between area to be investigated and surrounding tissue

This will get first mark

1

Barium meal proves high proton number / high density / high attenuation material at site to be investigated which provides much better contrast

This will gain the second mark

1

Barium meal proves high proton number / high density / high attenuation material at site to be investigated which provides much better contrast between area to be investigated and surrounding tissue

But this will get both marks

[7]

M2.(a) (i) Provide aperture through which X-rays may pass, stopping others ✓

Alternatives: provides collimation; produces narrow beam of X-rays; protects areas of the body not being scanned

1

- (ii) Filters out (most) low energy photons (but allows high energy photons to pass through) ✓

*Allow 'soft' or underpower' for low energy
Allow only high energy photons pass through*

1

- (b) $I / I_0 = 0.917$ ✓
 $\ln(0.917) = -\mu \times 2.7 \times 10^{-3}$ ✓
 $\mu = 32.1$ ✓
 $\mu_m = \mu / 2700 = 0.012$ ✓
 $\text{m}^2 \text{kg}^{-1}$ ✓

*If 0.083 or 91.7 used, final 3 calc marks can be given
If 0.83 or 8.3 or 9.17 used, final 2 calc marks can be given
Unit mark is independent mark*

5

[7]

- M3.** (a) for clear image need large difference in densities between part being investigated and parts around it **(1)**
when this is not natural, add material to part under investigation **(1)**
which has high density to provide good attenuation of X-rays **(1)**
barium meal use barium sulphate **(1)**

max 3

- (b) $\mu (= \rho\mu_m) = 2700 \times 0.012 = 32.4$ **(1)**
(use of $I = I_0 e^{-\mu x}$ gives) $1.2 \times 10^{-2} = 3.2 \times 10^{-2} \times e^{-32.4x}$ **(1)**
(allow C.E. for value of μ)
 $x = 0.03(0)$ m **(1)**

3

[6]

- M4.** (a) (i) converts X rays to visible photons **(1)**
(ii) converts photons to emission of electrons **(1)**

- (iii) increases kinetic energy of electrons travelling from cathode to anode **(1)**
focuses rays of electrons to produce faithful image **(1)**
- (iv) converts (increased) electron energy into light photons


max 4

- (b) dynamic process such as fluid flow **(1)**
cuts radiation dose whilst still providing good image
[or allows multiple or continuous use of X ray] **(1)**

2

[6]

- M5.(a)** (i) lead absorbs X-rays very well **(1)**

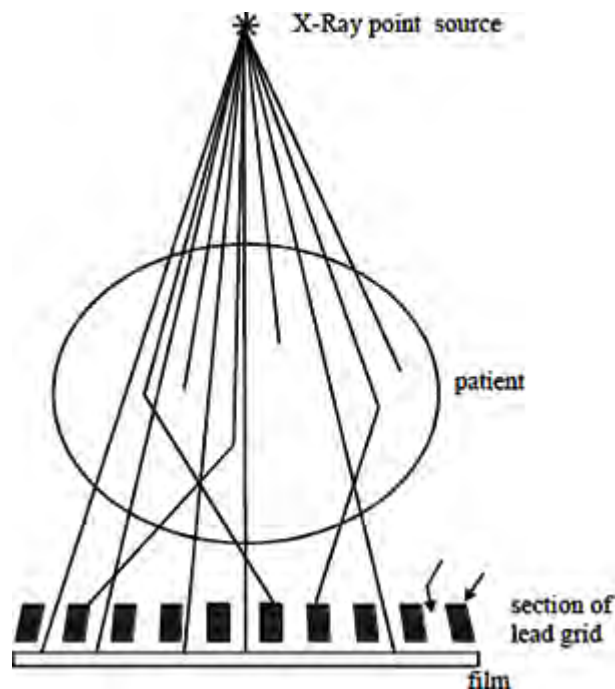

- (ii) straight through tracks **(1)**
scattered tracks absorbed by lead **(1)**
some X-rays absorbed by patient **(1)**
clarity lost if scattered rays reach film, darkening image in random places **(1)**

lead grid allows through to film only those rays which are not scattered
(1)
image intensity distribution represents accurately the body structure
through which the radiation has passed (1)
grid moved systematically to prevent it forming image on film

(max 5)

- (b) point source gives a sharp (shadow) image
[or point source produces no penumbra (grey fading at shadow edges) (1)

(1)

[6]

M6.(a) surface of body covered with an oil to improve transmission

from ultrasound transducer to body (1)

short ultrasound pulses sent into the body and echoes received

from surfaces detected by the transducer (1)

oscilloscope sweep time synchronised with the ultrasound pulse frequency (1)

(3)

- (b) (i) thickness = $\frac{1}{2} v \Delta t$ (1) = $\frac{1}{2} \times 1500 \times 0.08 \times 10^{-3}$ (m) (1)
= 0.06 m (1)

(ii) pulse duration = $0.3 \times 0.02 = 0.006$ m s (1)

(max 3)

(c) extra distance in tissue results in more signal absorption *

smaller fraction of signal reflected at second surface *

pulse more spread over time *

signal is diffracted *

* any two (1) (1)

(2)

